


Official partner of



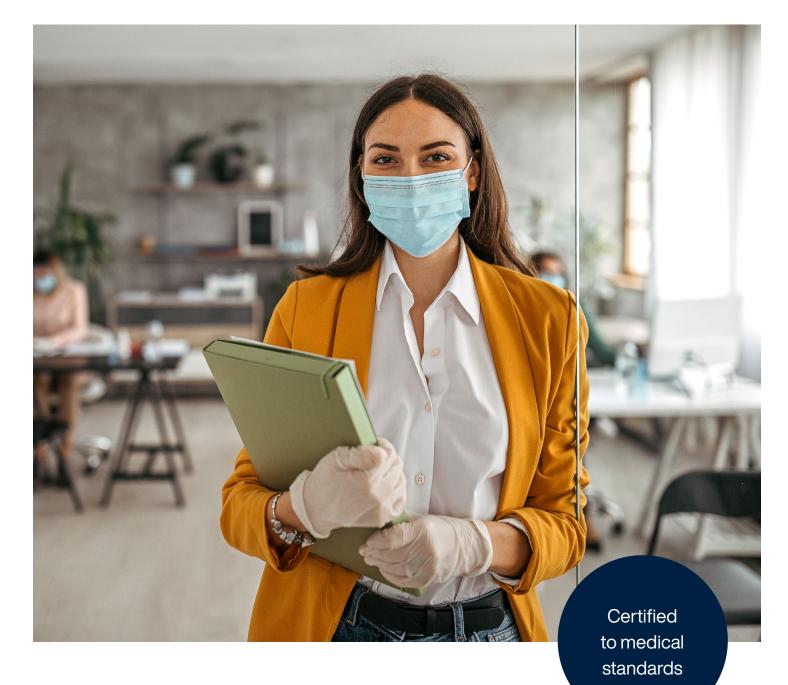

Health & Safety

Certified protective gloves



EXAMINATION GLOVE PORTFOLIO

HALYARD* GLOVES YOU'RE IN GOOD HANDS

INFECTION PREVENTION

O&M Halyard provides a full line of single-use infection control solutions to help reduce the spread of infections among patients and staff, from examination areas, to labs, to the OR[¥]. Included in this range are Facial Protection Solutions, Examination Gloves, Headwear, Footwear, Gowns and Scrub Suits.

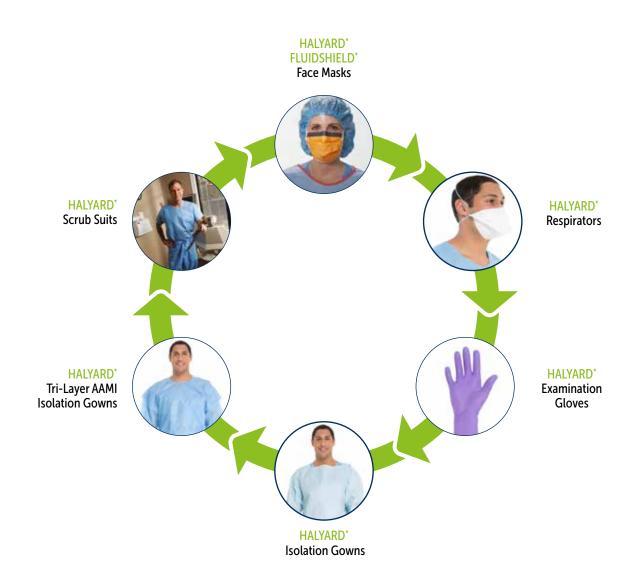




TABLE OF CONTENTS

| HALYARD'S NITRILE GLOVE PORTFOLIO | 4 |
|---|----|
| GLOVES PROPERTIES | 6 |
| CHEMOTHERAPY RESISTANCE BARRIER GUIDE | 6 |
| CHEMICAL RESISTANCE BARRIER GUIDE | 8 |
| PHYSICAL PROPERTIES | 10 |
| OTHER PRODUCT SPECIFICATIONS & QUALITY STANDARDS | 12 |
| EDUCATIONAL | 14 |
| GLOVES BY DEPARTMENT | 14 |
| SMARTPULL* DISPENSING | 16 |
| PROPER DONNING AND DOFFING OF NON-STERILE EXAM GLOVES | 17 |
| ITEM INDEX | 18 |



HALYARD'S NITRILE GLOVE PORTFOLIO OFFERING A GLOVE FOR EVERY NEED



PURPLE NITRILE* & PURPLE NITRILE* Sterile Exam Gloves

Maximum protection for high risk tasks or situations

PURPLE NITRILE^{*} Exam Gloves are frequently the glove choice for healthcare workers who need excellent barrier protection from bacteria, viruses and chemotherapy drugs. These durable gloves are available in 240, 310 and 400 mm lengths for maximum coverage and protection. Halyard's PURPLE NITRILE^{*} Exam Gloves are the original PURPLE NITRILE^{*} Gloves produced by Safeskin.



STERLING^{*} Nitrile Exam Gloves

Moderate risk tasks require a standard glove with STERLING^{*} reliability

STERLING^{*} Nitrile exam gloves were specifically designed to fit and feel like latex, with excellent comfort and tactile sensitivity. These gloves provide durable barrier protection and can be used facility-wide in a multitude of tasks. These gloves are available in 240 and 310 mm lengths for maximum coverage and protection (STERLING^{*} Nitrile-XTRA^{*}).



BASICS* Blue & BASICS* White Nitrile Exam Gloves

Low to moderate risk tasks require a cost effective glove that does not compromise on protection or comfort

BASICS^{*} Blue & BASICS^{*} White Nitrile exam gloves are thinner, lighter, and more economical than our standard nitrile gloves. The gloves are suitable for a wide range of tasks and are the ideal replacement for vinyl or latex exam gloves while maintaining comfort and fitting barrier protection during use.



BLACK-FIRE* Nitrile Exam Gloves

The functionality of two gloves in one

BLACK-FIRE^{*} Nitrile Exam gloves are reversible and can be used as a black glove or turned inside out to reveal the high-visibility, lower friction orange side.



Latex-Free Powder-Free Non-Sterile/Sterile Heavy-Weight

Chemotherapy drug tested >240 mm/ 310 mm/400 mm length



STERLING* Nitrile Facility-wide use

Latex-Free Powder-Free Non-Sterile Medium-Weight Cleaning chemical tested length

BASICS* Blue & BASICS* White Nitrile protection and comfort

Latex-Free Powder-Free Non-Sterile Light-Weight

Cost effective Comfortable Protective

>240 mm length



GLOVES PROPERTIES CHEMOTHERAPY RESISTANCE BARRIER GUIDE



The **HALYARD**^{*} **PURPLE NITRILE**^{*} **Examination glove family** are suitable for use with chemotherapy drugs. Our range of PURPLE NITRILE^{*} Examination Gloves have been tested according to the European norm EN374-1 and the US standard ASTM D6978. The HALYARD^{*} PURPLE NITRILE-MAX^{*} Gloves have been tested for use with more than 50 different chemotherapy drugs making it our most protective glove for use with cytoxic drugs.

| | PURPLE NITRILE* | PURPLE NITRILE-XTRA* | PURPLE NITRILE MAX* |
|-------------------------------|----------------------|----------------------|-------------------------|
| | Glove length >240 mm | Glove length 310 mm | Glove length >400mm |
| Chemotherapy Drugs | Breakthrough rating | Breakthrough rating | Breakthrough rating |
| Aresenic Trioxide (1 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Azacitidine (25 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Bendamustine (5 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Bortezomib (1 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Bleomycin sulfate (15 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Busulfan (6 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Carboplatin (10 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Carfilzomib (10 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Carmustine (3.3 mg/ml) | \oslash | \bigotimes | \bigotimes |
| Cetuximab (Erbitux) (2 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Cisplatin (1 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Cyclophosphamide (20 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Cytarabine HCL (100 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Cytovene (10 mg/ml) | NOT TESTED | \bigotimes | \bigotimes |
| Dacarbazine (10 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Daunorubicin HCL (5 mg/ml) | \bigotimes | \bigotimes | $\overline{\otimes}$ |
| Decitabine (5 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Docetaxel (10 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Doxorubicin HCL (2 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Ellence (2 mg/ml) | \bigotimes | \bigotimes | $\overline{\otimes}$ |
| Eribulin Mesylate (0.5 mg/ml) | \bigotimes | \bigotimes | $\overline{\otimes}$ |
| Etoposide (20 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Fludarabine (25 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Fluorouracil (50 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Fulvestrant (50 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Gemcitabine (38 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| ldarubicin (1 mg/ml) | \bigotimes | \bigotimes | \otimes |
| Ifosfamide (50 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Irinotecan (20 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Mechlorethamine HCL (1 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Melphalan (5 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |



| | PURPLE NITRILE* | PURPLE NITRILE-XTRA* | PURPLE NITRILE MAX* |
|--------------------------------|----------------------|-------------------------|-------------------------|
| | Glove length >240 mm | Glove length 310 mm | Glove length >400mm |
| Chemotherapy Drugs | Breakthrough rating | Breakthrough rating | Breakthrough rating |
| Methotrexate (25 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Mitomycin (0.5 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Mitoxantrone (2 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Oxaliplatin (2 mg/ml) | \bigotimes | \bigotimes | \bigotimes |
| Paclitaxel (6 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Paraplatin (10 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Pemetrexed (25 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Pertuzumab (30 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Raltitrexed (0.5 mg/ml) | NOT TESTED | \bigotimes | $\overline{\mathbf{O}}$ |
| Retrovir (10 mg/ml) | NOT TESTED | $\overline{\mathbf{O}}$ | $\overline{\mathbf{O}}$ |
| Rituximab (10 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Temsirolimus (25 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| ThioTEPA (10 mg/ml) | 0 | \bigotimes | $\overline{\mathbf{O}}$ |
| Topotecan HCL (1 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Trastuzumab (21 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Triclosan (1 mg/ml) | NOT TESTED | $\overline{\mathbf{O}}$ | $\overline{\mathbf{O}}$ |
| Trisenox (1 mg/ml) | \bigotimes | NOT TESTED | $\overline{\mathbf{O}}$ |
| Vinblastine (1 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Vincrinstine Sulfate (1 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Vinorelbine (10 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{O}}$ |
| Zoledronic Acid (0.8 mg/ml) | \bigotimes | \bigotimes | $\overline{\mathbf{N}}$ |

Rating Code

| Ø NOT RECOMMENDED | Avoid using this glove with this chemical |
|-------------------|--|
| | This glove is suitable for this chemical under careful control of its use (breakthrough time < 59 min) |
| ♦ RECOMMENDED | This glove is well suited for use with this chemical (breakthrough time > 60 min) |
| NOT TESTED | - |

PURPLE NITRILE*: The following chemotherapy drugs and concentrations showed breakthrough detected in less than 30 minutes. Carmustine (3.3 mg/ml): 1.8 minutes ThioTEPA (10.0 mg/ml): 1.6 minutes. Warning: Not for use with Carmustine and ThioTEPA Caution: The testing conditions used are intended to approximate the worst case conditions for clinical use. Testing was conducted on single layer glove material. It is the users' responsibility to adapt the applicability of the these gloves for their intended use with the cited chemotherapy drugs. Breakthrough time data available on request.

CHEMICAL RESISTANCE BARRIER GUIDE

The **HALYARD' STERLING' Nitrile and PURPLE NITRILE' Examination Gloves** are tested for use with various chemical substances according to EN 374-1 and ASTM F739-12, thereby ensuring our customers are always informed and adequately protected when working with potentially hazardous chemicals.

| | STERLING* Nitrile | PURPLE NITRILE* | PURPLE NITRILE-XTRA* |
|---|--------------------------|--------------------------|--------------------------|
| | Glove length >240 mm | Glove length >240 mm | Glove length 310 mm |
| Chemical | Breakthrough rating | Breakthrough rating | Breakthrough rating |
| Adhesive Tape Remover Pads | $\underline{\mathbb{V}}$ | \bigotimes | \otimes |
| Alcoholic Bouin's Fixative | $\underline{\mathbb{V}}$ | \bigotimes | \otimes |
| Alcoholic Eosin | $\underline{\mathbb{V}}$ | \triangle | Λ |
| Bleach | \otimes | \otimes | \otimes |
| Bouin's Fixative | \bigotimes | \bigotimes | \otimes |
| B-Plus Fixative | \bigotimes | \bigotimes | \otimes |
| CarNoy's Fluid | 0 | \oslash | 0 |
| Chlorhexidine Gluconate 4% | NOT TESTED | \otimes | \otimes |
| Cidex 14-Day | \bigotimes | \bigotimes | \otimes |
| Cidex OPA | \otimes | \bigotimes | \otimes |
| Decalcifier I | \bigotimes | \bigotimes | \otimes |
| EM Fixative | \otimes | \bigotimes | \otimes |
| Eosin Stain | $\underline{\mathbb{V}}$ | \bigotimes | \otimes |
| Ethidium Bromide (1%) | \otimes | \bigotimes | \otimes |
| Ethyl Alcohol (95%) | $\underline{\mathbb{V}}$ | $\underline{\mathbb{V}}$ | $\underline{\mathbb{V}}$ |
| Formalin Alcohol (tested for Formaldehyde) | ۸ | Δ | \otimes |
| Formalin Alcohol (tested for Reagent Alcohol) | Δ | \otimes | \otimes |
| Formalin, 10% Buffered (tested for Formaldehyde) | \otimes | \otimes | \otimes |
| Formalin, 10% Buffered (tested for Methanol) | \otimes | \otimes | \otimes |
| Giemsa Stain Solution | $\underline{\mathbb{V}}$ | $\underline{\mathbb{V}}$ | $\underline{\mathbb{V}}$ |
| Glutaraldehyde 4% | \otimes | \otimes | \otimes |
| Haematoxylin Stain (Harris Solution) | \otimes | Δ | \otimes |
| Hydrochloric Acid, 35.5% | \otimes | \otimes | \otimes |
| Hydrogen Peroxide, 3% | \otimes | \bigotimes | \otimes |
| Isopropyl Alcohol, 70% | $\underline{\mathbb{V}}$ | Δ | \otimes |



| | STERLING [*] Nitrile | PURPLE NITRILE* | PURPLE NITRILE-XTRA* |
|--|-------------------------------|----------------------|--------------------------|
| | Glove length >240 mm | Glove length >240 mm | Glove length 310 mm |
| Chemical | Breakthrough rating | Breakthrough rating | Breakthrough rating |
| Methanol | ${\mathbb A}$ | \square | $\underline{\mathbb{V}}$ |
| Methyl Methacrylate (Bone Cement) | 0 | 0 | Δ |
| Monsel's Solution | \bigotimes | \bigotimes | \bigotimes |
| OxyCide Concentrate | ${\mathbb A}$ | \bigotimes | \bigotimes |
| OxyCide Ready to Use | \bigotimes | \bigotimes | \bigotimes |
| Permaslip Mounting Medium & Liquid Cover Slip | 0 | 0 | 0 |
| Rapid Bone Decalcifier | \bigotimes | \bigotimes | \bigotimes |
| Reagent Alcohol | Δ | Λ | Δ |
| Resert XL HLD | Δ | \bigotimes | \bigotimes |
| Sodium Hydroxide (40%) | $\overline{\mathbf{O}}$ | \bigotimes | \bigotimes |
| Trichloroacetic Acid, (10%) | $\overline{\mathbf{O}}$ | \bigotimes | \bigotimes |
| Xylene, 99% | \bigcirc | 0 | 0 |
| Acetone | Δ | \wedge | \wedge |
| Ethyl Acetate | Δ | \wedge | \wedge |
| n-Heptane | $\overline{\mathbf{N}}$ | \bigotimes | \bigotimes |
| Sulphuric Acid (96%) | \mathbb{A} | \wedge | \wedge |
| Nitric acid (65%) | Δ | \wedge | \wedge |
| Acetic acid (99%) | \mathbb{A} | \wedge | \wedge |
| Ammonium Hydroxide (25%) | Δ | Λ | \wedge |
| Hydrogen Peroxide (30%) | Δ | \bigotimes | \bigotimes |
| Formaldehyde (37%) | $\overline{\mathbf{O}}$ | \bigotimes | \bigotimes |
| Incidin Rapid (Isopropanol) | NOT TESTED | \bigotimes | NOT TESTED |
| Incidin Foam (Isopropanol & Ethanol) | NOT TESTED | \otimes | NOT TESTED |
| Incidin Plus (Diethylene Glycol Butyl Ether & phenoxyethanol) | NOT TESTED | \otimes | NOT TESTED |


Rating Code

| Ø NOT RECOMMENDED | Avoid using this glove with this chemical |
|-------------------|--|
| | This glove is suitable for this chemical under careful control of its use (breakthrough time < 59 min) |
| | This glove is well suited for use with this chemical (breakthrough time > 60 min) |
| NOT TESTED | - |


These gloves are not intended for applications involving direct exposure to harsh chemicals, where heavy-duty industrial gloves are required. It is the users' responsibility to adapt the applicability of the these gloves for their intended use with the cited chemicals. Breakthrough time data available on request.

PHYSICAL PROPERTIES

Force at break is an indication of the strength of the glove. It measures the force (Newton) required in order to break a glove by stretching it. EN455-2 requires that nitrile examination gloves meet a minimum force at break of 6N. The HALYARD^{*} STERLING^{*} Nitrile & PURPLE NITRILE^{*} Examination Glove families all exceed the minimum force at break requirement. Our BASICS^{*} Blue & BASICS^{*} White Nitrile Examination Gloves comply to the norm with a 6N force at break.

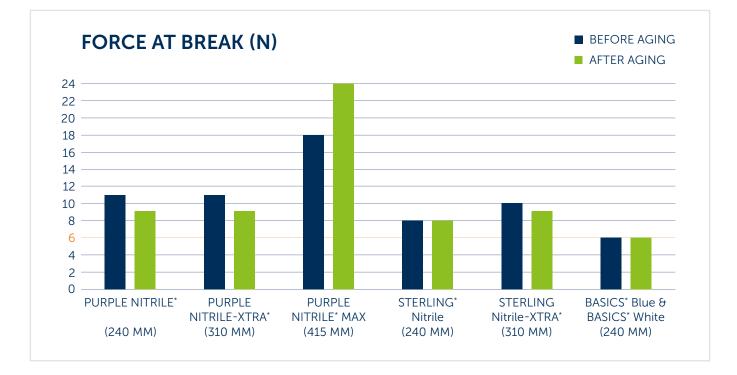


EN455-1 describes a method in which randomly sampled gloves are subjected to a water tightness test, i.e. the ability of a glove to hold 1000ml of water without leaking. For compliance to the EN 455-1, the Acceptance Quality Limit (AQL) should be 1.5. The HALYARD* STERLING* Nitrile & PURPLE NITRILE* Examination Glove families all exceed (in terms of performance), the Acceptance Quality Limit with an AQL 1.0. Our BASICS* Blue & BASICS* White Nitrile Examination Gloves maintain an AQL 1.5.

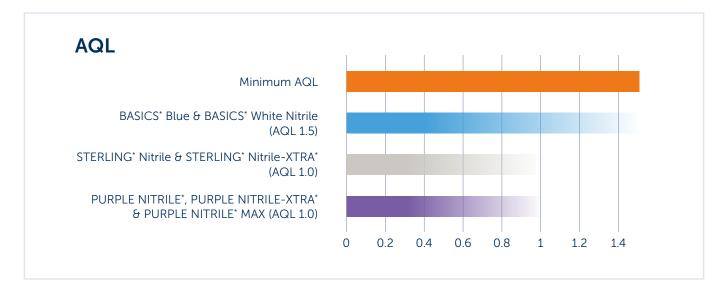



Palm Thickness is a metric that can be used in determining both tactile sensitivity and barrier protection. Consistency for this metric is key for both durability and chemical permeation protection. The below chart indicates the palm thickness of HALYARD^{*} gloves per glove family.

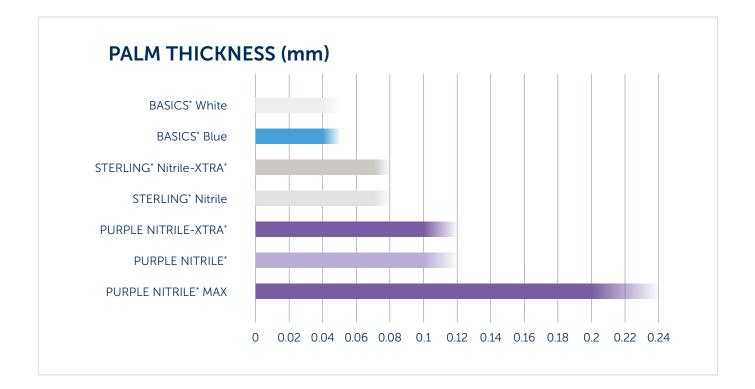

OTHER PRODUCT SPECIFICATIONS & QUALITY STANDARDS

| Gauge thickness measurements | | | | |
|------------------------------|--------------------|-------------------------|------------------------------------|----------------------|
| | W | | | |
| | PURPLE NITRILE* | PURPLE NITRILE-XTRA* | PURPLE NITRILE [*] MAX | STERLING* Nitrile |
| Middle finger | 0.15 mm | 0.15 mm | 0.28 mm | 0.09 mm |
| Palm | 0.13 mm | 0.12 mm | 0.24 mm | 0.08 mm |
| Cuff | 0.09 mm | 0.11 mm | 0.15 mm | 0.06 mm |
| Average length | > 240 mm | 310 mm | 415 mm | > 240 mm |

| Product specifications - Palm width | | | | | |
|-------------------------------------|-------------------|-------------------------|------------------------------------|----------------------|--|
| | | | | | |
| | PURPLE NITRILE | PURPLE NITRILE-XTRA* | PURPLE NITRILE [*] MAX | STERLING* Nitrile | |
| X-Small | 70 mm | 70 mm | - | 70 mm | |
| Small | 80 mm | 80 mm | 80 mm | 80 mm | |
| Medium | 95 mm | 95 mm | 100 mm | 95 mm | |
| Large | 110 mm | 110 mm | 111 mm | 110 mm | |
| X-Large | 120 mm | 120 mm | 121 mm | 120 mm | |

| Quality standards | | | | | | | |
|--|--------------|--------------|--------------|------------------|----------------------------|--|---|
| | EN 455 | EN 374 | EN 420 | PPE (Cat III) | Approved for food handling | CE mark as per 93/42/EEC Directive for Medical Devices | Quality system (manufacturing sites) |
| PURPLE NITRILE [*] | ✓ | \checkmark | \checkmark | ✓ | - | Class of device: I | ISO 13485 and ISO 9001 compliant |
| PURPLE NITRILE-XTRA* | ✓ | \checkmark | \checkmark | ✓ | - | Class of device: I | ISO 13485 and ISO 9001 compliant |
| PURPLE NITRILE [*] MAX | ✓ | \checkmark | \checkmark | ✓ | - | Class of device: I | ISO 13485 and ISO 9001 compliant |
| PURPLE NITRILE [*] Sterile | \checkmark | - | - | - | - | Class of device: I - sterile | ISO 13485 and ISO 9001 compliant |
| STERLING [*] Nitrile | ✓ | \checkmark | \checkmark | ✓ | \checkmark | Class of device: I | ISO 13485 and ISO 9001 compliant |

Gauge thickness measurements

| | STERLING* Nitrile-XTRA | BASICS [*] Blue & BASICS [*] White | BLACK-FIRE* |
|----------------|---------------------------|---|-------------|
| Middle finger | 0.11 mm | 0.07 mm | 0.14 mm |
| Palm | 0.08 mm | 0.05 mm | 0.10 mm |
| Cuff | 0.07 mm | 0.04 mm | 0.09 mm |
| Average length | 310 mm | > 240 mm | > 240 mm |

| Product specifications - Palm width | | | | |
|-------------------------------------|---------------------------|---|-------------|--|
| | | | | |
| | STERLING Nitrile-XTRA* | BASICS [®] Blue & BASICS [®] White | BLACK-FIRE* | |
| X-Small | 70 mm | 75 mm | 70 mm | |
| Small | 80 mm | 85 mm | 80 mm | |
| Medium | 95 mm | 95 mm | 95 mm | |
| Large | 110 mm | 106 mm | 110 mm | |
| X-Large | 120 mm | 116 mm | 120 mm | |

| Quality standards | | | | | | | |
|---|--------|--------------|--------------|------------------|----------------------------|--|---|
| | EN 455 | EN 374 | EN 420 | PPE (Cat III) | Approved for food handling | CE mark as per 93/42/EEC Directive for Medical Devices | Quality system (manufacturing sites) |
| STERLING Nitrile-XTRA* | ✓ | \checkmark | \checkmark | ✓ | \checkmark | Class of device: I | ISO 13485 and ISO 9001 compliant |
| BASICS [•] Blue & BASICS [•] White | ✓ | \checkmark | \checkmark | ✓ | \checkmark | Class of device: I | ISO 13485 and ISO 9001 compliant |
| BLACK-FIRE* | ✓ | \checkmark | \checkmark | \checkmark | \checkmark | Class of device: I | ISO 13485 and ISO 9001 compliant |

EDUCATIONAL GLOVES BY DEPARTMENT

Choosing the correct glove based on the risk of the anticipated task is crucial in a healthcare worker's daily activities.

| Chemotherapy administration - Critical care - Ambulance | | | | | | | | |
|---|----------------------------------|----------------------------|--------------------|-------------------------|--|--|--|--|
| High risk tasks typically require a high risk glove | | | | | | | | |
| BASICS [*] Blue & BASICS [*] White | STERLING [*] Nitrile | STERLING* Nitrile-XTRA* | PURPLE NITRILE* | PURPLE NITRILE-XTRA* | PURPLE NITRILE [*] Sterile | | | |
| - | - | - | \checkmark | \checkmark | - | | | |

| Labour/OBGYN - Dermatology - Wound care - Minor non-invasive procedures - Burn units | | | | | | | | |
|--|----------------------------------|----------------------------|--------------------------------|------------------------|--|--|--|--|
| High risk tasks typically require a high risk glove | | | | | | | | |
| BASICS [*] Blue & BASICS [*] White | STERLING [*] Nitrile | STERLING* Nitrile-XTRA* | PURPLE NITRILE [*] | PURPLE NITRILE-XTRA | PURPLE NITRILE [*] Sterile | | | |
| - | - | - | - | - | \checkmark | | | |

| Facility-wide use - ICU - OR - Pharmacies - Laboratories | | | | | | | | |
|---|----------------------------------|--|--------------------------------|-------------------------|--|--|--|--|
| Moderate risk tasks may require a standard glove with Sterling* reliability | | | | | | | | |
| BASICS [*] Blue & BASICS [*] White | STERLING [*] Nitrile | STERLING [*] Nitrile-XTRA* | PURPLE NITRILE [*] | PURPLE NITRILE-XTRA* | PURPLE NITRILE [*] Sterile | | | |
| \checkmark | ✓ | \checkmark | \checkmark | \checkmark | - | | | |

| Phlebotomy - General patient care & transportation - Routine oral care | | | | | | | | |
|--|---|--|--------------------|-------------------------------------|--|--|--|--|
| Low risk t | Low risk tasks often require a cost effective glove that does not compromise on protection or comfort | | | | | | | |
| BASICS [*] Blue & BASICS [*] White | STERLING* Nitrile | STERLING [*] Nitrile-XTRA [*] | PURPLE NITRILE* | PURPLE NITRILE-XTRA [*] | PURPLE NITRILE [*] Sterile | | | |
| \checkmark | ✓ | \checkmark | \checkmark | - | \checkmark | | | |

The tasks listed serve as examples of typical use, however, it is ultimately up to the end user to identify and choose the most appropriate glove for the task they will undertake.



SMARTPULL* DISPENSING



The HALYARD^{*} SMARTPULL^{*} Exam Glove box has two openings to allow for better glove dispensing and less waste!

The system features two separate openings on the box. The first, smaller opening is used when the box is full to reduce multiple dispensing, which often results in exam glove waste when gloves become unusable after falling on the floor. When the box is half empty, the second, larger opening allows for easier access to the gloves.

The patented dispensing technology is featured on our PURPLE NITRILE*, STERLING* Nitrile, BASICS* Blue & BASICS* White Nitrile Examination Glove boxes.

DIRECTIONS FOR USE



STEP 1 Remove the perforated carton opening at Tab 1



The smaller opening helps prevent multiple dispensing and glove waste.



STEP 2

As the box empties and it becomes difficult to reach inside, remove the opening indicated by Tab 2



Continue dispensing as you would from a traditional glove carton.

PROPER DONNING AND REMOVAL OF NON-STERILE EXAM GLOVES

DONNING -



Before donning your gloves, always wash your hands.



Take out a glove from its original dispenser, holding only the cuff.

REMOVAL -



Using your dominant hand. Grasp the outside cuff of your opposite gloved hand and peel the glove off. This turns the glove inside out.



Hold the removed glove in your gloved hand.



Hold the glove at its opening with one hand and slide your fingers and thumb of the opposite hand into the glove.



Take a second glove out of the dispenser with your bare hand, holding only the cuff.



Pull the glove towards your wrist to fully don the glove. Only use your knuckles while doing this to avoid fingernail punctures.



Hold the glove at its opening and slide your fingers and thumb into the glove. Pull the glove towards your wrist using the knuckles of your gloved hand.



Slide two fingers of your ungloved hand under the remaining glove cuff at your wrist.



Discard your gloves in the appropriate waste container or garbage can.



Peel the second glove off your hand turning it inside out and enclosing the first glove within it.



After you dispose of your gloves, wash your hands thoroughly.

ITEM INDEX

| ITEM INDEX | | | | | | | |
|--|---------------------------------|-------------------|--------|--------|--------|---------|--|
| Description | Packaging | Item code by size | | | | | |
| | | X-Small | Small | Medium | Large | X-Large | |
| PURPLE NITRILE | 100 gloves/box 10 boxes/case | 52000M | 52001M | 52002M | 52003M | | |
| Exam Gloves | 90 gloves/box 10 boxes/case | | | | | 52004M | |
| PURPLE NITRILE-XTRA* Exam Gloves | 50 gloves/box 10 boxes/case | 50600M | 50601M | 50602M | 50603M | 50604M | |
| PURPLE NITRILE* MAX | 50 gloves/box 8 boxes/case | | 47195 | 47196 | 47197 | 47198 | |
| PURPLE NITRILE [*] Sterile Exam Gloves | 50 gloves/box 4 boxes/case | | 52201M | 52202M | 52203M | | |
| STERLING [*] Nitrile | 200 gloves/box 10 boxes/case | 13938 | 13940 | 13941 | 13942 | | |
| Exam Gloves | 170 gloves/box 10 boxes/case | | | | | 13943 | |
| STERLING [*] ZERO Nitrile | 200 gloves/box 10 boxes/case | 47471 | 47472 | 47473 | 47474 | | |
| Accelerator Free Exam Gloves | 170 gloves/box 10 boxes/case | | | | | 47475 | |
| STERLING [*] Nitrile-XTRA [*] Exam Gloves | 100 gloves/box 10 boxes/case | 44286 | 44287 | 44288 | 44289 | 44290 | |
| BASICS* Blue Nitrile | 200 gloves/box 10 boxes/case | 44749 | 44750 | 44751 | 44752 | | |
| Exam Gloves | 170 gloves/box 10 boxes/case | | | | | 44753 | |
| BASICS' White Nitrile | 200 gloves/box 10 boxes/case | 44740 | 44741 | 44742 | 44743 | | |
| Exam Gloves | 170 gloves/box 10 boxes/case | | | | | 44744 | |
| | 150 gloves/box 10 boxes/case | 45256 | 45257 | 45258 | 45259 | | |
| BLACK-FIRE* | 140 gloves/box 10 boxes/case | | | | | 45260 | |



Climate Protection for Future Growth

Innovating since 1946



Our products and services

GoGaS specializes in heating, cooling, ventilation and UV-C disinfection. We offer innovative solutions that address environmental, decarbonization, health and safety challenges and safety.

We'll always be glad to help you!

Building climate

Air Distribution Systems Heat Pumps Heat Recovery High Intensity Heaters HVLS Fans Hydrogen Burners LED Lighting Technology Patio Heaters Regulation Technology Solar Air Systems Tube Heaters Ventilation Systems Warm Air Heaters

Process Solutions

De-icing systems Drying Technologies Process Heat Recycling Technologies

Health & Safety

Protective Equipment UV-C Ambient Air Disinfection UV-C Building Disinfection UV-C Surface Disinfection

> Nachhaltig wirtschaftlich effizient



Certified:

DAkkS Deutsche Akkreditierungsstelle D-ZM-17431-01-01 BLUECOMPETENCE Alliance Member Partner of the Engineering Industry Sustainability Initiative

Partner:

GoGaS Goch GmbH & Co. KG

Zum Ihnedieck 18 44265 Dortmund Germany

T +49 231 46505-0 F +49 231 46505-88

protect@gogas.com www.gogas.com

